

**COMPACT LOW TEMPERATURE
SCANNING PROBE MICROSCOPES**

**COMPACT LOW TEMPERATURE
SCANNING PROBE MICROSCOPES**



PPMS[®] SPM

Compact Low Temperature Scanning Probe Microscopes

© 2010, attocube systems AG - Germany. attocube systems and the logo are trademarks of attocube systems AG. Registered and/or otherwise protected in various countries where attocube systems products are sold or distributed. Other brands and names are the property of their respective owners.

attocube systems AG | Königinstrasse 11a (Rgb) | D - 80539 München | Germany
Tel.: +49 89 2877 809 - 0 | Fax: +49 89 2877 809 - 19 | info@attocube.com
www.attocube.com

 **attocube systems**
explore your nanoworld

 **attocube systems**
explore your nanoworld

01 SCANNING PROBE MICROSCOPY

FOR THE QUANTUM DESIGN PPMS®

attocube systems' scanning probe microscope family (CFM, AFM, MFM, SNOM*, and STM*) has undergone a redesign to fit any 25 mm (1") static sample space including the Quantum Design PPMS®. Despite the compactness, all microscopes provide a coarse travel range of 3 x 3 x 2.5 mm³ and a scan range of 12 x 12 μm² at low temperature (4 K). The outstanding stability of the microscopes allows investigation of nm-sized structures with highest resolution making these instruments versatile tools for state-of-the-art research on the nanometer scale.

attocube systems and Quantum Design have announced a strategic partnership to promote and distribute attocube's new scanning probe microscopes designed specifically for the PPMS® of Quantum Design. This collaboration expands technology reach and provides both new and existing PPMS® customers with easier access to additional measurement and characterization techniques.

With the SPM insert for the Physical Property Measurement System (PPMS®) of Quantum Design, attocube meets growing demands for highly sophisticated yet easy-to-use scanning probe microscopes.



The ultra-compact, high resolution PPMS®-SPM uses advanced technologies such as low temperature compatible objectives for confocal microscopy or a fiber-optical interferometer for force microscopy with outstanding signal-to-noise force detection. The rugged housing construction is made from highest quality Titanium, ensuring maximum stability and minimum sample drift during variation of temperature and/or magnetic field. The patented driving technology of the coarse positioning system warrants a precise and reliable sample approach and positioning in three axes with nanometer precision over several millimeters range. Plus, the instrument is fully

compatible with commercially available AFM / MFM cantilevers.


In combination with the Quantum Design PPMS® with its broad temperature and magnetic field range, stability and ease of use, exciting new measurements are only some clicks away ...

THE NEXT LEVEL PPMS SOLUTION


THE ONLY SCANNING PROBE MICROSCOPES FOR THE PPMS® CERTIFIED & ENDORSED BY QUANTUM DESIGN.

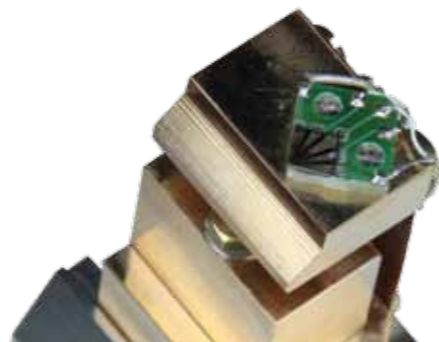

Magnetic Force Microscopy (MFM)



Scanning Hall Probe Microscopy (SHPM)



Atomic Force Microscopy (AFM)



Confocal Microscopy (CFM)

attoAFM xs
ultra-stable, compact atomic force microscope with interferometric deflection detection for highest stability and sensitivity. Compatible with contact and non-contact AFM mode.

attoMFM xs
ultra-stable, compact magnetic force microscope with interferometric deflection detection for highest stability and sensitivity. Compatible with dual-pass and constant height MFM mode.

attoCFM xs
ultra-stable, compact confocal microscope based on fiber or free-beam optics for maximum flexibility and stability.

attoSHPM xs
ultra-stable, compact scanning Hall probe microscope with STM tracking 2DEG Hall sensor for maximum field sensitivity.

* available on request.


02 attoMFM Ixs

LOW TEMPERATURE MAGNETIC FORCE MICROSCOPE



The attoMFM Ixs is an ultra-compact magnetic force microscope designed particularly for applications at low and ultra low temperature. On the basis of a conventional atomic force microscope, the instrument works by scanning a sample below a fixed magnetic cantilever. The magnetic force gradient acting on the tip is then determined by measuring the change in resonance frequency (FM mode) or phase of the cantilever (AM mode) with highest precision using a fiber-based optical interferometer. Both measurement modes are applied at a certain tip-sample distance, typically around 10 - 100 nm. In FM mode, a phase-locked loop (PLL) is used to excite the cantilever at resonance.

Principle - The microscope uses a set of xyz-positioners for coarse positioning of the sample over a range of several mm. Developed particularly for cryogenic applications, the piezo scanner ANSxy50 provides a scan range of 12 x 12 μm^2 even at liquid helium temperature. The adjustment of the MFM cantilever is performed outside of the cryostat prior to cooling down the microscope. The exceptional combination of materials allows absolutely stable high resolution imaging of surfaces.


04

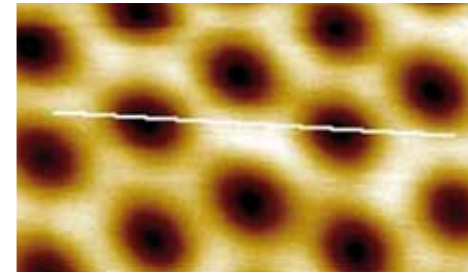

06

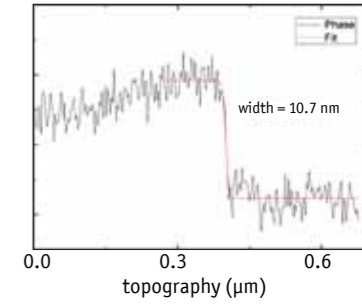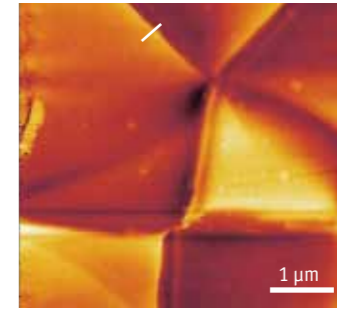

05

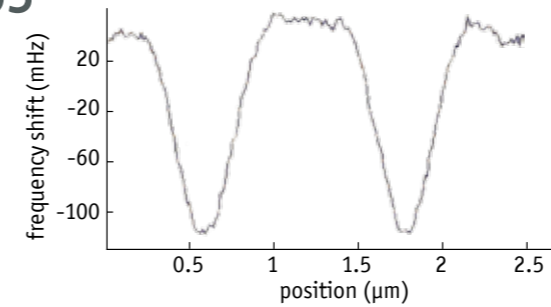


Results

04. Hexagonal vortex lattice in optimum doped Bi-2212 at a temperature of 4.1 K and a magnetic field of 45 Gauss. The image shows unprocessed, as-measured MFM phase data recorded at 70 nm constant height.

05. Line scan of the above shown vortex lattice in optimum doped Bi-2212.

06. MFM measurement on 300 nm NiFe Pads showing their magnetic structure. The image was recorded at 300 K with 20 nm tip-sample separation in dual-pass mode, yielding a spatial resolution of 10.7 nm and a phase contrast of 2.3 degrees

01

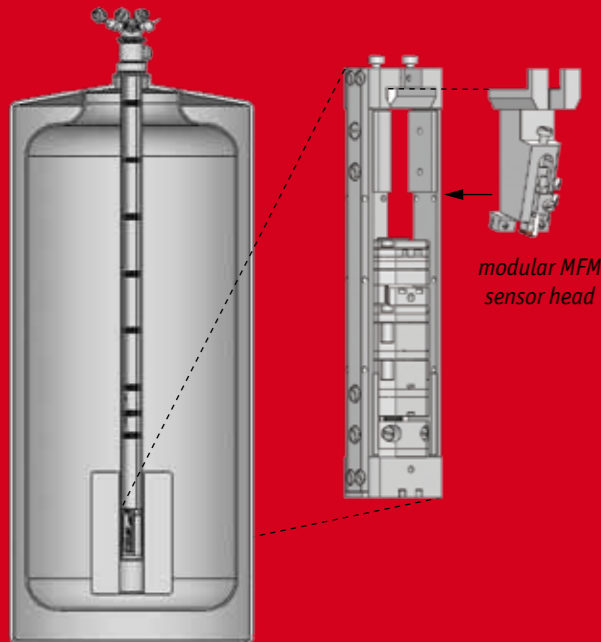

01. Schematic drawing of the low temperature attoMFM Ixs and the surrounding PPMS dewar.

02. The attoMFM Ixs microscope module.

03. ASC500 iBox - manual control unit for the ASC500 SPM controller.

02



03



Specifications

Operation Mode	feedback imaging modes coarse range	PI feedback loop with additional PLL contact mode, non-contact mode, high-resolution MFM mode, EFM, SGM 3 x 3 x 2.5 mm ³
Sample Positioning	step size scan range temperature range	@ 300 K: 0.025 .. 2 μm 30 x 30 x 5 μm^3 1.9 .. 400 K (full PPMS [®] temperature range) @ 4 K: 10 .. 500 nm 12 x 12 x 2 μm^3
Operating Conditions	magnetic field range operating pressure	0 .. 16 T (full PPMS [®] magnetic field range) 1E-6 mbar .. 1 bar (designed for exchange gas atmosphere)
Resolution	control electronics lateral (xy) bit resolution at 300 K z bit resolution at 300 K lateral (xy) bit resolution at 4 K z bit resolution at 4 K MFM resolution at 300 K and 4 K	16 bit over selected scan range (virtually unlimited bit resolution) 0.46 nm at 30 μm scan range 0.075 nm at 5 μm scan range 0.18 nm at 12 μm scan range 0.03 nm at 2 μm scan range 20 nm
Sample Size		10 x 10 x 5 mm ³ max.

03 attoSHPM xs

LOW TEMPERATURE SCANNING Hall PROBE MICROSCOPE

The attoSHPM xs is an ultra-compact scanning Hall probe microscope, designed particularly for the operation at low temperature and high magnetic fields. At the heart of the SHPM, a molecular beam epitaxy (MBE) grown GaAs/AlGaAs Hall sensor measures magnetic fields with unrevealed sensitivity. Local measurements of the magnetization of a sample are obtained by scanning the sample underneath the Hall sensor and simultaneously recording the Hall voltage, directly yielding the local magnetic field. While other local probes may outperform the Hall sensor with respect to its lateral resolution, its ability to non-invasively obtain quantitative values for the local magnetic field makes the Hall sensor a unique tool for the study of superconductors and other magnetic materials.


Principle - The microscope uses a set of xyz-positioners for coarse positioning of the sample over a range of several mm. The scanning motion of the sample is provided by an ANSxy50 piezo scanner, providing a scan range of $12 \times 12 \mu\text{m}^2$ at 4.2 K. The adjustment of the Hall sensor is performed outside of the cryostat prior to cooling down the microscope. The exceptional combination of materials allows absolutely stable high resolution imaging of surfaces/local magnetic fields.

01

01. Schematic drawing of the low temperature attoSHPM xs and the surrounding PPMS dewar.

02. Close-up of the attoSHPM xs microscope module.

03. Photograph of the attoSHPM xs microscope head, showing the Hall chip and its carrier (green). The tilt angle of the Hall sensor with respect to the sample can be arbitrarily adjusted between 0° and approximately 5° .

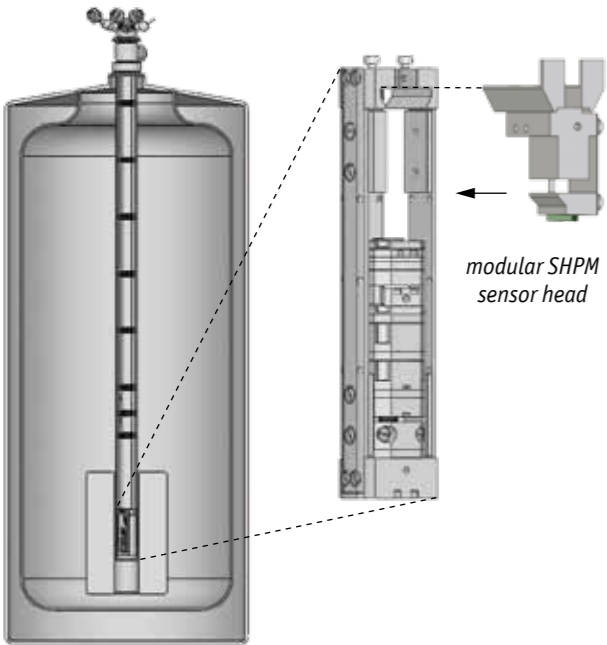


modular SHPM sensor head



02



03

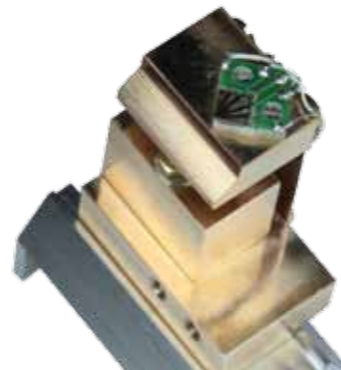


04

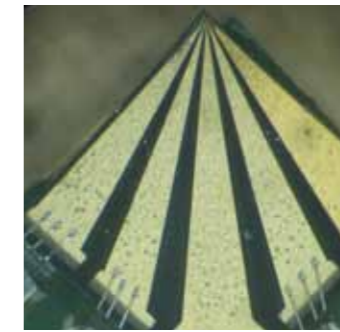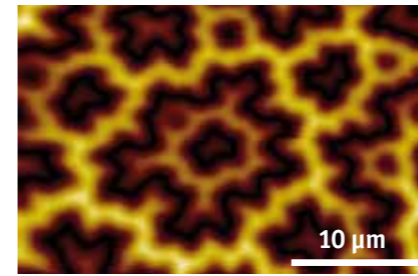

Close-up of the MBE grown SHPM chip, showing its Hall-sensor/STM leads and the bond wires for electrical connection to the chip carrier. The Hall sensors are available as high resolution and ultra-high resolution versions, featuring an active Hall area of 500 nm and 300 nm, respectively.

05

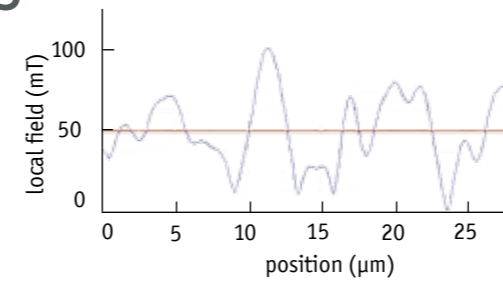

Results

04. SHPM image of BaFeO, recorded at a 4.2 K in constant height mode. The color scale spans 106 mT (black to white), while the S/N ratio of this measurement yields 2×10^{-5} T.

05. Line scan over the complete SHPM scan of BaFeO, recorded at 4.2 K in constant height mode.

Specifications

Operation Mode	feedback imaging modes coarse range	STM tracking distance detection, tuning fork tracking on request STM tracking, constant height, or dual pass mode $3 \times 3 \times 2.5 \text{ mm}^3$
Sample Positioning	step size scan range temperature range	@ 300 K: 0.025 .. 2 μm 30 x 30 x 5 μm^3 1.9 .. 400 K (full PPMS® temperature range) @ 4 K: 10 .. 500 nm 12 x 12 x 2 μm^3
Operating Conditions	magnetic field range operating pressure	0 .. 16 T (full PPMS® magnetic field range) 1E-6 mbar .. 1 bar (designed for exchange gas atmosphere)
Resolution	control electronics lateral (xy) bit resolution at 300 K z bit resolution at 300 K lateral (xy) bit resolution at 4 K z bit resolution at 4 K	16 bit over selected scan range (virtually unlimited bit resolution) 0.46 nm at 30 μm scan range 0.075 nm at 5 μm scan range 0.18 nm at 12 μm scan range 0.03 nm at 2 μm scan range
Hall Sensor	design active area field sensitivity	MBE grown GaAs/AlGaAs heterostructure 500 nm (high resolution) 300 nm (ultra high resolution) 1500 V/AT
Sample Size		10 x 10 x 5 mm^3 max.

04 attoAFM Ixs

LOW TEMPERATURE ATOMIC FORCE MICROSCOPE

The attoAFM Ixs is an ultra-compact atomic force microscope designed particularly for applications at low and ultra low temperature. The instrument works by scanning a sample below a fixed cantilever while measuring its deflection with highest precision using a fiber based optical interferometer. Combined with the ASC500 SPM controller, both contact and non-contact modes are applicable, making the attoAFM Ixs a powerful tool for topographic measurements, force spectroscopy and other imaging modes. Apart from these capabilities, the superior mechanical stability of the measurement head allows an operation inside of cryogen free pulse-tube based cooling systems, providing access to applications where liquid Helium is not available or not desired.

Principle - The microscope uses a set of xyz-positioners for coarse positioning of the sample over a range of several mm. Developed particularly for cryogenic applications, the piezo scanner ANSxy50 provides a scan range of $12 \times 12 \mu\text{m}^2$ even at liquid helium temperature. The adjustment of the cantilever is performed outside of the cryostat prior to cooling down the microscope. The exceptional combination of materials allows absolutely stable high resolution imaging of surfaces.


PRODUCT KEY FEATURES

- > ultra compact AFM head
- > highly sensitive interferometric deflection detection
- > unreached mechanical stability
- > adjustment of the cantilever outside of the cryostat prior to cooling the microscope
- > in-situ, long range positioning at low temperature


BENEFITS

- > fits standard cryogenic and magnet sample spaces
- > high resolution AFM imaging
- > quick sample and cantilever exchange
- > highest stability in variable magnetic fields
- > highest stability at variable temperature
- > offers all common contact and non-contact modes (contact, intermittent contact, true non-contact)
- > interferometric deflection detection
- > large scan range at low temperature
- > designed to work seamlessly with the QD PPMS®
- > large range, patented coarse positioning system
- > patented coarse positioning driving technology

04

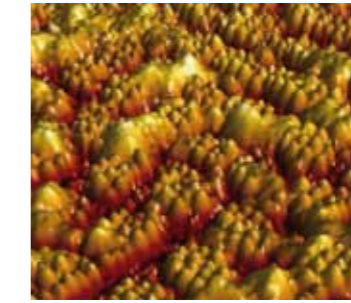

05

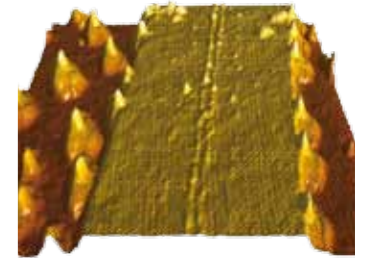


Results

04. AFM contact mode image of an ordered lattice of InAs quantum dot molecules recorded at 4.2 K (attocube application labs, 2007).

05. AFM contact mode image of a layered Si/SiO₂-Substrate (height: 20 nm +/- 2 nm) recorded at 4.2 K. Height of surface contaminations: ~ 1 nm. (attocube application labs 2007).

01

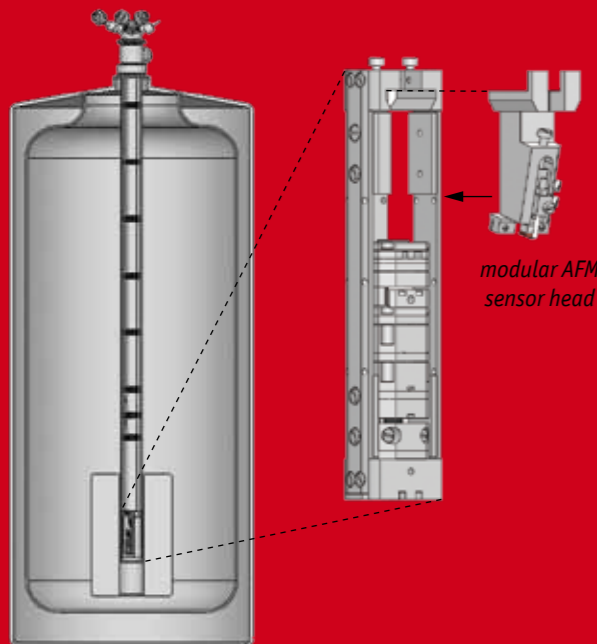

modular AFM sensor head

01. Schematic drawing of the low temperature attoAFM Ixs and the surrounding PPMS dewar.

02. Close-up of the attoAFM Ixs microscope module.

03. ASC500 - attocube's state-of-the-art Scanning Probe Microscopy controller featuring an open architecture and high flexibility to meet the customers' individual needs.

02



03



Specifications

Operation Mode	feedback imaging modes coarse range	PI feedback loop with additional PLL contact mode, non-contact mode, EFM, SGM, PRFM, ... 3 x 3 x 2.5 mm ³
Sample Positioning	step size scan range temperature range	@ 300 K: 0.025 .. 2 μm 30 x 30 x 5 μm ³ 1.9 .. 400 K (full PPMS® temperature range) @ 4 K: 10 .. 500 nm 12 x 12 x 2 μm ³
Operating Conditions	magnetic field range operating pressure	0 .. 16 T (full PPMS® magnetic field range) 1E-6 mbar .. 1 bar (designed for exchange gas atmosphere)
Resolution	control electronics lateral (xy) bit resolution at 300 K z bit resolution at 300 K lateral (xy) bit resolution at 4 K z bit resolution at 4 K	16 bit over selected scan range (virtually unlimited bit resolution) 0.46 nm at 30 μm scan range 0.075 nm at 5 μm scan range 0.18 nm at 12 μm scan range 0.03 nm at 2 μm scan range
Sample Size		10 x 10 x 5 mm ³ max.

05 attoCFM xs

LOW TEMPERATURE CONFOCAL MICROSCOPE

The attoCFM xs has been developed to offer highest flexibility combined with maximum mechanical stability for low temperature confocal microscopy experiments. The attoCFM xs can be ordered with either free-beam or fiber based optics. In case of the free-beam optics, excitation and collection ports are completely independent, allowing the introduction of further optical components (e.g. filter or polarizer) and enabling measurements such as Raman spectroscopy. Offering slightly less flexibility, the fiber based setup is designed for highest mechanical stability allowing single quantum dot measurements over a timespan of several weeks and operation in cryogen-free cryostats.

Principle - The microscope uses a set of xyz-positioners for coarse positioning of the sample over a range of several mm. Developed particularly for cryogenic applications, the piezo scanner ANSxy50 provides a scan range of $12 \times 12 \mu\text{m}^2$ even at liquid helium temperature. The exceptional combination of materials allows absolutely stable high resolution imaging of surfaces.


PRODUCT KEY FEATURES

- > ultra compact CFM head
- > fiber based or free-beam optics
- > fully adjustable excitation and collection ports (free-beam)
- > wavelength or polarization filtering (free-beam)
- > ultra-stable design (fiber based)
- > in-situ, long range positioning at low temperature


BENEFITS

- > fits 1" clear bore cryostats and magnets
- > highest flexibility and sensitivity combined with minimal light loss
- > access to optical spectroscopy such as Raman spectroscopy (free-beam)
- > highly stable long term measurements

04

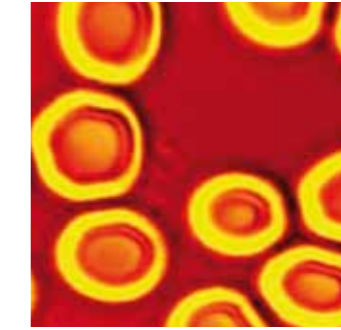

05

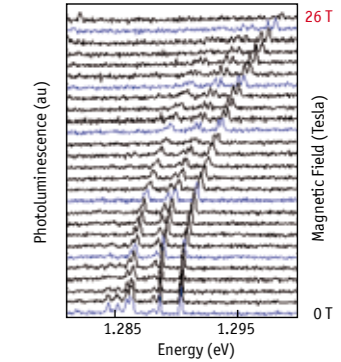

Results

04. Confocal image of red blood cells fixed on a glass slide. The image was recorded with the fiber based CFM in reflection mode (scan voltage 30 V).

05. Photoluminescence spectroscopy of a single quantum dot as exposed to magnetic fields of up to 26 T.


Specifications

01

01. Schematic drawing of the low temperature attoCFM xs and the surrounding PPMS dewar.

02. Close-up of the attoCFM xs microscope module.

03. attocube offers various low temperature compatible objectives with different numerical apertures and working distances.

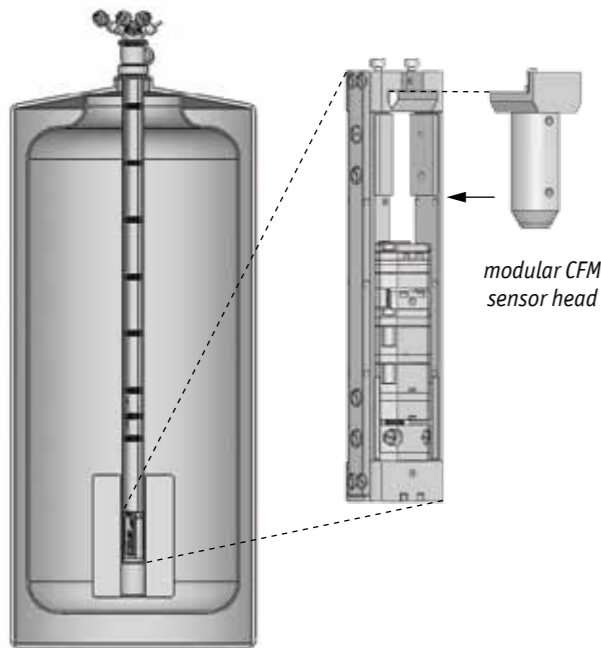

modular CFM sensor head

02



03



Microscope configuration

confocal unit

ultra-stable and compact confocal microscope head
fiber optic or free-beam based
illumination / collection fiber (blocking pinhole)

Sample Positioning

step size
scan range
temperature range

@ 300 K: 0.025 .. 2 μm @ 4 K: 10 .. 500 nm
30 x 30 x 5 μm^3 12 x 12 x 2 μm^3
1.9 .. 400 K (full PPMS[®] temperature range)

Operating Conditions

magnetic field range
operating pressure

0 .. 16 T (full PPMS[®] magnetic field range)
1E-6 mbar .. 1 bar (designed for exchange gas atmosphere)

Illumination

excitation wavelength range
light source
light power on the sample
port specification

~400 .. 1500 nm (see objectives description)
fiber coupled laser (typically 400 .. 1500 nm)
typically 1 pW .. 500 μW
FC/APC-connector for single mode fibers (other connector types on request)

Sample Size

10 x 10 x 5 mm³ max.

06 ASC500

FULLY DIGITAL SPM CONTROLLER



The ASC500 is a modular and flexible digital SPM controller which combines state-of-the-art hardware with innovative software architecture, offering superior performance and an unprecedented variety of control concepts. The ASC500 controller was developed with the goal to never be the limiting factor in any SPM experiment. All desirable functions and high-end specifications for conducting the experiment of your choice in MFM, SHPM, AFM, CFM, SNOM, STM, and many more are available.

Are you missing the sensitive adjustment possibilities provided by former analog SPM-units? Every ASC500 can be equipped with the ASC-iBox unit allowing fast and controlled manual adjustment of all major parameters. Now you are able to combine the advantages of manual and software control of your experiments.

Scan Engine:

The ASC500 uses a dedicated hardware with a 5 MHz scan generator to create the voltages necessary for the raster motion. The 16 bits of the xy outputs are always automatically mapped to the actual scan field, yielding a virtually unlimited bit resolution.

Z controller:


The z scanner output is controlled by a digital PI algorithm with a bandwidth of 50 kHz. The z output DAC has a resolution of 18 bit, yielding a 4 pm resolution on a 1 μm scan range. This resolution can be increased to a theoretical value of 60 attometer by limiting the control range.

PLL

A fully digital phase locked loop is implemented into the ASC500. It uses the high frequency inputs/outputs with 50 MHz bandwidth. A high-speed Lock-in demodulator and two PI control loops are used to control the amplitude of an oscillator and to follow any shifts in resonance. The frequency resolution is below 0.2 μHz in a range of 1 kHz up to 2 MHz.



STATE-OF-THE-ART CONTROLLER (ASC500)

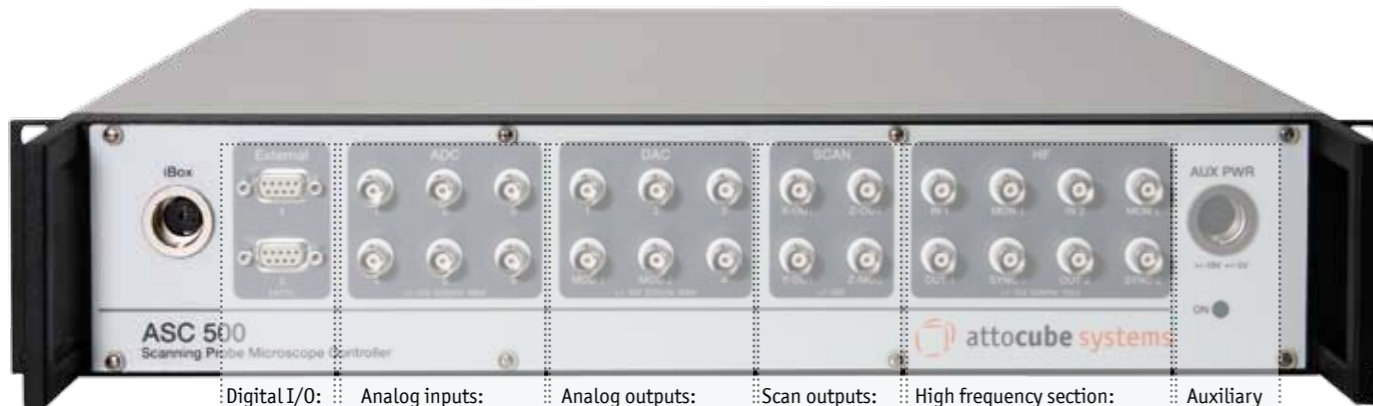

Digital I/O:	Analog inputs:	Analog outputs:	Scan outputs:	High frequency section:	Auxiliary power:
8 inputs 8 outputs 40 MHz	6 converters 400 kHz 18 bit	4 converters 200 kHz 16 bit 2 analog modulation inputs	3 converters 5 MHz in xy; highest resolution, z modulation input	2 independent HF channels with each: 50 MHz 16 bit input 50 MHz 16 bit output Sync output Pre-amplified signal monitor	+/- 5 V +/- 15 V



Q Control

The ASC500 provides full control over the Q factor of any driven lever system by means of electronic Q control. The natural Q factor of the lever can be varied by typically more than one order of magnitude in each direction (increase/decrease).

LabVIEW™ control

The new LabVIEW™ interface provides full control over all ASC500 functions. Benefits are: measurement automatization, user definable experiments, and easy implementation with 3rd party instrumentation.


Spectroscopy

The ASC500 features advanced spectroscopy techniques such as z spectroscopy and bias voltage spectroscopy. These measurements are supported by an internal Lock-in and a limiter functionality which drastically reduces the likelihood of a tip crash. Spectroscopy measurements can be automatically triggered on line, grid, or point-by-point paths. Combinations of spectroscopies can be defined in action lists.


07

ATTOCUBE SYSTEMS' CONTROLLER


OPEN UP NEW POSSIBILITIES

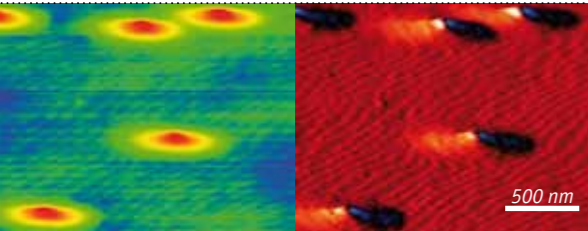

The internal PLL of the ASC500 was used to control a high Q tuning fork AFM. Topography measurements were performed on uncapped, stacked InAs Quantum Dots in a GaAs matrix. The evaluation of the height distribution revealed atomic steps with a spacing of ~ 2 Ångstrom. Topography and error signal were recorded simultaneously.

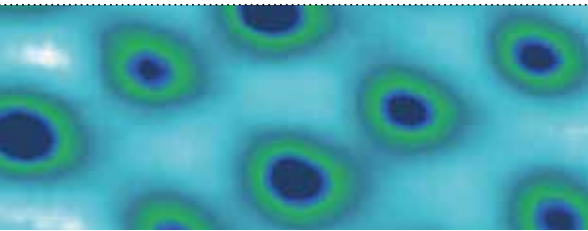

A cantilever based low temperature MFM was used to image single vortices on BSCCO. The signal quality could be significantly enhanced by using the Q control functionality of the ASC500. The Q factor of the MFM lever was increased by a factor of 4 to record this image. For non-flat surfaces, dual pass mode can be employed for highest magnetic resolution.

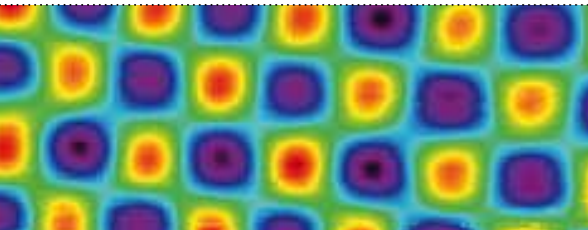

The ASC500 provides a step scan function to gain unlimited scan range at low temperatures. The above image was taken using a confocal microscope on a test grating. The raster motion was achieved by single step coarse movement of xy positioners. The ASC500 controls the coarse movement and synchronizes data collection.

The ANC350 is attocube's multi-functional piezo controller which meets the highly demanding dynamic performance and accuracy requirements of multi-axis nanopositioning setups. The real-time operating system enables the closed loop control of attocube's nanopositioners with optoelectronic and resistive encoders. All functionalities are accessible via USB 2.0 or an optional Ethernet port.



The ANC250 is a dedicated, ultra low noise scan voltage amplifier for piezo scanning tubes and flexure scanners. With an output noise of $150 \mu\text{V}_{\text{pp}}$ in 500 kHz bandwidth, the ANC250 offers the lowest noise specs on the market. Its three input channels drive five bipolar output channels with an amplification of ± 20 . The output voltages ($x+$, $x-$, $y+$, $y-$, z) of up to ± 200 V are ideally suited to drive piezo tube scanners.



08

ATTOCUBE SYSTEMS

CREATING SCIENTIFIC IMPACT

S. Gröblacher, J. B. Hertzberg, M. R. Vanner, G. D. Cole, S. Gigan, K. C. Schwab, M. Aspelmeyer
Demonstration of an ultracold micro-optomechanical oscillator in a cryogenic cavity
Nature Physics 5, 485–488 (2009).

B.D. Gerardot, D. Brunner, P.A. Dalgarno, P. Öhberg, S. Seidl, M. Kroner, K. Karrai, N.G. Stoltz, P.M. Petroff, R.J. Warburton
Optical pumping of a single hole spin in a quantum dot
Nature 451, 441–444 (2008).

M. Kroner, A.O. Govorov, S. Remi, B. Biedermann, S. Seidl, A. Badolato, P.M. Petroff, W. Zhang, R. Barbour, B.D. Gerardot, R.J. Warburton, K. Karrai
The nonlinear Fano effect
Nature 451, 311–314 (2008).

M. Kroner, C. Lux, S. Seidl, A.W. Holleitner, K. Karrai, A. Badolato, P.M. Petroff, R.J. Warburton
Rabi splitting and ac-Stark shift of a charged exciton
Appl. Phys. Lett. 92, 031108 (2008).

M. Ediger, G. Bester, A. Badolato, P.M. Petroff, K. Karrai, A. Zunger, R.J. Warburton
Peculiar many-body effects revealed in the spectroscopy of highly charged quantum dots
Nature Physics 3, 774–779 (2007).

B.D. Gerardot, S. Seidl, P.A. Dalgarno, R.J. Warburton, M. Kroner, K. Karrai, A. Badolato, P.M. Petroff
Contrast in transmission spectroscopy of a single quantum dot
Appl. Phys. Lett. 90, 041101 (2007).

I. Favero, C. Metzger, S. Camerer, D. König, H. Lorenz, J.P. Kotthaus, K. Karrai
Optical cooling of a micromirror of wavelength size
Appl. Phys. Lett. 90, 104101 (2007).

B.D. Gerardot, S. Seidl, P.A. Dalgarno, R.J. Warburton, D. Granados, J.M. Garcia, K. Kowalik, O. Krebs
Manipulating exciton fine structure in quantum dots with a lateral electric field
Appl. Phys. Lett. 90, 041101 (2007).

A. Babiński, G. Ortner, S. Raymond, M. Potemski, M. Bayer, W. Sheng, P. Hawrylak, Z. Wasilewski, S. Fafard, A. Forchel
Ground-state emission from a single InAs/GaAs quantum dot structure in ultrahigh magnetic fields
Phys. Rev. B 74, 075310 (2006).

M. Atatüre, J. Dreiser, A. Badolato, A. Högele, K. Karrai, A. Imamoglu
Quantum-Dot Spin-State Preparation with Near-Unity Fidelity
Science, 312(5773), 551 (2006).

A. Högele, S. Seidl, M. Kroner, K. Karrai, M. Atatüre, J. Dreiser, A. Imamoglu, R. J. Warburton, B. D. Gerardot, P. M. Petroff
Spin-selective optical absorption of singly charged excitons in a quantum dot
Appl. Phys. Lett. 86, 221905 (2005).

M. Kroutvar, Y. Ducommun, D. Heiss, M. Bichler, D. Schuh, G. Abstreiter, J. Finley
Optically programmable electron spin memory using semiconductor quantum dots
Nature, 432, 81 (2004).

K. Karrai, R.J. Warburton, C. Schulhauser, A. Högele, B. Urbaszek, E. J. McGhee, A. O. Govorov, J. M. Garcia, B. D. Gerardot, P. M. Petroff
Hybridization of electronic states in quantum dots through photon emission
Nature, 247, 135 (2004).

A. Högele, S. Seidl, M. Kroner, K. Karrai, R. J. Warburton, B. D. Gerardot, P. M. Petroff
Voltage-Controlled Optics of a Quantum Dot
Phys. Rev. Lett., 93, 217401 (2004).

A. Babinski, S. Awirothananon, J. Lapointe, Z. Wasilewski, S. Raymond, M. Potemski
Single-Dot Spectroscopy in High Magnetic Fields
Physica E, 22, 603 (2004).

R. J. Warburton, C. Schäfflein, D. Haft, F. Bickel, A. Lorke, K. Karrai, J. M. Garcia, W. Schoenfeld, P. M. Petroff
Optical emission from a charge-tunable quantum ring
Nature 405, 926 (2000).